

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):


- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problems Mailbox.**

INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification ⁵ : A61M 15/00	A1	(11) International Publication Number: WO 93/17728 (43) International Publication Date: 16 September 1993 (16.09.93)
(21) International Application Number: PCT/EP93/00473 (22) International Filing Date: 3 March 1993 (03.03.93) (30) Priority data: 92850046.1 4 March 1992 (04.03.92) EP (34) Countries for which the regional or international application was filed: PT et al. (71) Applicant (for all designated States except US): AKTIEBOLAGET ASTRA [SE/SE]; S-151 85 Södertälje (SE). (72) Inventors; and (75) Inventors/Applicants (for US only): KÄLLSTRAND, Göran [SE/SE]; Dragonvägen 1, S-237 00 Bjärred (SE). NILSSON, Per-Gunnar [SE/SE]; Danska Vägen 35, S-212 14 Malmö (SE).		(74) Agents: LINDEROTH, Margareta et al.; AB Astra, Patent Department, S-151 85 Södertälje (SE). (81) Designated States: AT, AU, BB, BG, BR, CA, CH, CZ, DE, DK, ES, FI, GB, HU, JP, KP, KR, LK, LU, MG, MN, MW, NL, NO, NZ, PL, PT, RO, RU, SD, SE, SK, UA, US, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, ML, MR, SN, TD, TG). Published <i>With international search report.</i> <i>Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i>

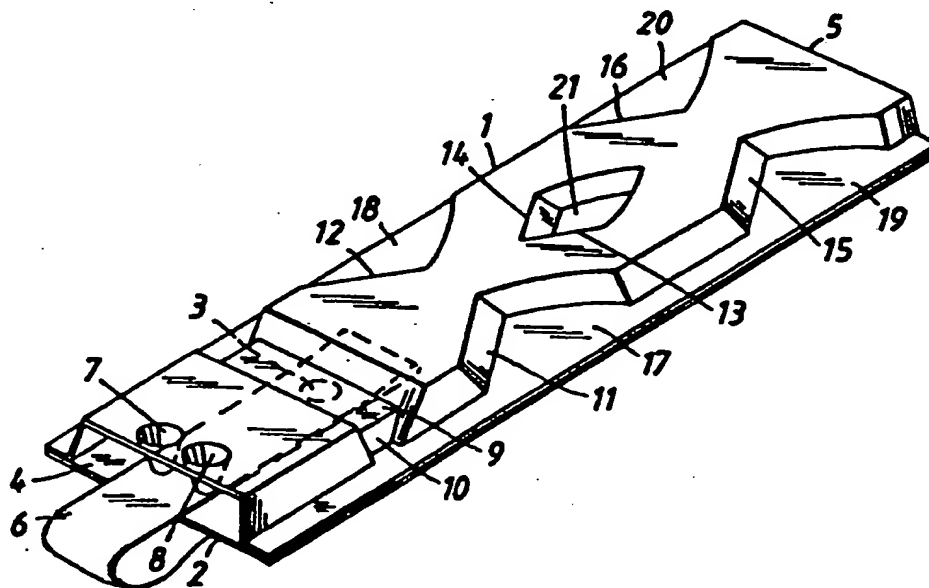(54) Title: DISPOSABLE INHALER II**(57) Abstract**

The invention relates to a disposable breath-actuated inhaler comprising a tubular housing forming an air flow path being open at both ends, one end forming an air inlet (4) and one end forming an air outlet (5), said housing comprising a compartment (3) for storing a pharmaceutical powder to be inhaled. The compartment (3) for storing the pharmaceutical powder is located close to the air inlet (4) and is covered by a thin foil (6) sealing the compartment in an airtight way which can be removed from the compartment from outside the housing, said housing being shaped with a constriction (9) adjacent the powder compartment (3) such that a turbulent air stream will be obtained at the constriction upon inhalation which will lift the powder out from the compartment (3) and mix the powder into the air stream.

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	FR	France	MR	Mauritania
AU	Australia	GA	Gabon	MW	Malawi
BB	Barbados	GB	United Kingdom	NL	Netherlands
BE	Belgium	GN	Guinea	NO	Norway
BF	Burkina Faso	GR	Greece	NZ	New Zealand
BG	Bulgaria	HU	Hungary	PL	Poland
BJ	Benin	IE	Ireland	PT	Portugal
BR	Brazil	IT	Italy	RO	Romania
CA	Canada	JP	Japan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SK	Slovak Republic
CI	Côte d'Ivoire	LJ	Liechtenstein	SN	Senegal
CM	Cameroon	LK	Sri Lanka	SU	Soviet Union
CS	Czechoslovakia	LU	Luxembourg	TD	Chad
CZ	Czech Republic	MC	Monaco	TG	Togo
DE	Germany	MG	Madagascar	UA	Ukraine
DK	Denmark	ML	Mali	US	United States of America
ES	Spain	MN	Mongolia	VN	Viet Nam
FI	Finland				

DISPOSABLE INHALER II5 Technical field of the invention.

The present invention relates to a breath-actuated disposable inhaler of the kind having a generally tubular shape and having two ends, one end forming an
10 air inlet and one end forming an air outlet, the inhaler containing a pharmaceutical powder comprising particles of a respirable size which is to be inhaled.

15 Background of the invention.

Disposable, breath-actuated inhalers of the kind described above are for instance disclosed in WO 89/01348, US-A-4,265,236 and EP-A-0404454.

20

EP-A-0404454 discloses a disposable, breath-actuated inhaler comprising a chamber for a pharmaceutical powder, said chamber being provided with an air inlet and with an air outlet. The air inlet and outlet are
25 covered by a common cover. The powder is disposed loosely in said comparatively large chamber which means that the powder not necessarily will be located at that location at which the air flow is most efficient.

30 US-A-4,265,236 discloses a tubular disposable, breath-actuated inhaler comprising a flexible tube, the ends of which normally being sealingly inserted into each other. This kind of seal will not necessarily be moisture-proof. There furthermore is a risk that some
35 amount of the powder may fall out of the inhaler when the ends of the tube are pulled apart.

WO 89/01348, in the embodiment most of interest here, discloses a tubular, disposable inhaler which is sealed in both ends by means of twist-off caps. The pharmaceutical powder is loosely disposed in the inhaler and, as in the other inhalers described above, there is a risk that some powder is lost when the inhaler is opened.

The objects of the invention are to provide a disposable inhaler of the kind described above in which the dose of pharmaceutical powder can be determined accurately and in which the pharmaceutical powder can be stored hermetically sealed and moisture-proof. The dose delivered by different specimens of the same inhaler should generally be constant. The inhaler finally should be easy to prepare for use and easy to use as well as being easy and cheap to manufacture.

Brief description of the inventive concept.

The above objects are achieved in that the disposable inhaler is provided with the features set forth in the appended main claim. Advantageous embodiments are set forth in the dependent claims.

Brief description of the appended drawings.

Fig 1 shows a perspective view of an inhaler according to the invention,
Fig 2 shows a perspective view of an inhaler according to Fig 1 but showing the two main parts of the inhaler in an unassembled state,
Figs 3A - 3C show different stages in the opening of the powder compartment of the inhaler of Fig 1,

Fig 4 shows an end view of the air inlet of the inhaler in Fig 1,

Figs 5 - 7 show different possible embodiments of the constriction adjacent the powder compartment.

5

Detailed description of a preferred embodiment of the invention.

10 A preferred embodiment of the invention is disclosed in Figs 1 - 4. In Fig 1 the inhaler can be seen in a fully assembled condition and ready for use. As can be seen, the inhaler essentially comprises two elongate main parts, an upper part 1 which is made of a moulded sheet
15 of plastic material and a lower part 2 preferably made of aluminium foil laminated with plastic. The upper part 1 is U-shaped with a substantially rectangular shape. The width of the upper part is several times the height. The lower part is generally flat and the two
20 parts thus form a tubular housing defining an air conduit or air flow path with an air inlet 4 and an air outlet 5. A part-spherical depression or recess 3 indicated with a dashed line is located close to the air inlet 4. The recess 3 forms a powder compartment
25 and is covered by a tape 6 which preferably is made of aluminium foil, also laminated with plastic. The recess 3 may also be provided with one or several small through-holes 24 in the bottom. The hole or holes 24 should be large enough to allow the entry of air into
30 the recess from the underside of the lower part, but
----- sufficiently small to prevent any part of the powder from falling out through the hole(s).

As indicated, the end of the part of the tape 6
35 covering the recess 3 is located between the recess 3 and the air inlet 4. The tape is attached to the lower part 2 around the powder compartment by means of a

relatively weak weld 22 which can be seen in Fig 2. The end of the tape is attached by a comparatively large and thus stronger weld in front of the compartment, as seen in the intended direction of the air flow. The free part of the tape 6 is bent backwards over the recess 3 and extends out through the air inlet 4. In this particular embodiment, the free part of the tape is guided and held by two conical projections 7,8 extending downwards from the upper part 1. The free part of the tape may be bent in a loop to the underside of the lower part 2 and attached to the lower part all around the recess 3 by a relatively weak weld, thus sealing the hole 24 and the recess 3. The tape should be sufficiently long to extend past the recess 3, thus forming a tab 25 to serve as a grip for tearing the tape away.

A constriction in the flow path in the form of a ridge 9 oriented perpendicularly relative to the direction of the flow path is located above the powder compartment. The ridge is formed as a depression 9 in the upper part 1. The ridge is delimited at each end by an abutment 10.

The inhaler is further provided with deaggregation means after the powder compartment, as seen in the direction of the intended air flow through the inhaler. These deaggregation means comprise a number of oblique planar surfaces which are oriented at an angle of about 30° relative to the longitudinal direction of the inhaler, it surprisingly having been found that the most efficient angle of a planar surface relative to the air flow direction for disintegrating powder agglomerations is about 30°. Since the air flow will be deflected to some extent by the planar surface, the flow direction will not coincide fully with the longitudinal direction, but the above angle has been

chosen as being the best compromise. The angle can however be varied between 20° and 50° with a preferred range of 25° - 35°.

5 The planar surfaces are oriented generally
perpendicularly relative to the lower part 2, or at
least as perpendicularly as the method of manufacturing
the inhaler allows. The planar surfaces are located in
such a way that their projections onto a cross-
10 sectional plane substantially cover the entire cross-
section of the inhaler. The projections preferably
should overlap to some extent in order to ensure that
any larger particles or agglomerations entrained in the
air flow will impact on at least one such surface. In
15 the preferred embodiment the planar surfaces 11, 12,
13, 14, 15, 16 are located on the upstream ends of two
pairs of indentions 17, 18; 19, 20, formed into the
sides of the upper part 1 and on the upstream end of a
central depression 21 located between said indentations
20 forming an island in the flow path. The downstream ends
of said indentations and said depression taper in the
direction of the air flow and have a smooth, rounded
shape in order to obtain good aerodynamic conditions
without any areas where the powder entrained in the air
25 flow could settle.

The two main parts of the inhaler are shown separated
in Fig 2. Apart from the details shown in Fig 1, the
powder compartment 3 is shown opened, the tape 6 having
30 been pulled outwardly through the air inlet. The shape
of the ~~-(broken)~~ weld 22 can be seen on the tape 6 and
around the powder compartment 3. As can be seen, the
shape of the weld has been chosen to be the perimeter
of a square oriented with one diagonal parallel with
35 the longitudinal extent of the inhaler. This means that
the disengagement of the tape from the lower part 2
will be facilitated since the tearing action will both

start and end at a corner. Since the weld holding the inner end of the tape is broad and strong, the user will feel when the compartment has been uncovered by means of the increased resistance.

5

Figs 3A - 3C show different stages in the opening of the powder compartment 3 by pulling the tape 6, thus exposing the powder 23. Fig 3A shows the tape 6 attached around the recess 3 on the under side of the lower part, thus covering the hole 24 whilst leaving a tearing tab 25.

10

The end view is shown in Fig 4 more clearly illustrates the inter-relationship between the upper part 1, the lower part 2, the powder compartment 3, the tape 6, the conical projections 7, 8, the ridge 9 and the abutments 10.

15

When the inhaler is to be used, the inhaler is held more or less horizontal with the flat half 2 facing downwards. The free end of the tape 6 is pulled by means of the tab 25, thus exposing the hole 23 and the powder in the powder compartment 3. The two conical projections 7, 8 will hold the tape 6 flat against the lower part 2 and thus prevent the tape from occluding the constriction in front of the powder compartment. The user then inserts the air outlet into the mouth and inhales through the inhaler. The resultant air flow through the inhaler will become very turbulent in the region of the constriction and the pharmaceutical powder will be lifted out of the powder compartment and mixed with the air flow. Any particles adhering to the tape may also be entrained with the air flow since the part of the tape originally covering the powder compartment also will lie directly in the flow path. By admitting air into the bottom of the recess 3, the through-hole 24 will counteract any subpressures in the

20

25

30

35

bottom of the recess which might impede the lifting of the powder out of the recess.

5 Tests have shown that the dose leaving a typical powder compartment (e.g. about 0.5 mg) located at a constriction having an area of about 10 - 12 mm² will remain essentially constant at air flow rates varying from 30 l/min to 60 l/min.

10 The powder-laden air will then flow from the constriction to the deaggregation means. The angle of attack of the oblique surfaces will entail that the lighter particles, i. e. the particles within the respirable range, < 6µm, will be deflected from the
15 surface without sticking thereto and thus mainly will follow the air flow, whereas the heavier particles and agglomerates will impact on and rebound from the planar surfaces and in this way be broken up into smaller particles. As mentioned above, an angle of about 30°
20 may be optimal.

In this case tests again have shown that the percentage of particles within the respirable range in the dose to be inhaled will remain substantially constant at air
25 flow rates ranging from 30 l/min to 60 l/min.

That the dose of respirable particles remains substantially constant over a wide range of air flows is important in order to minimize the difference
30 between patients with different inhalation capacities.

It should be noted that the tubular shape of the inhaler makes it possible to mount a rubber ball or similar over the air inlet. By the means thereof the
35 powder could be ejected from the inhaler into the throat of the patient in synchronization with the breathing of the patient by a helper if the patient

should be incapable to use the inhaler by himself.

As mentioned above, the lower part 2 of the inhaler as well as the tape 6 preferably are made of aluminium foil laminated or coated with a suitable plastic. The aluminium will ensure the desired protection against moisture whereas the plastic will ensure that the tape can be welded to the lower part and that the lower part can be welded to the upper part. The lower part may for instance consist of a aluminium foil having a thickness of 45 μ which on one side is covered with a layer of oriented polyamide which is 25 μ thick and on the other side is covered by a layer of polypropene which is 60 μ thick. The upper part is preferably made of polypropene being 300 or 400 μ thick. The upper part can be transparent so that the user can see if the dose has been ejected from the powder compartment.

The tape may be made of a laminate having a "peel"-effect comprising polyester, aluminium and a layer comprising a polymer mixture of polybuten and polypropene.

The choice of material in the inhaler should be adapted to the drug to be used. The above materials have been chosen with a specific drug (budesonide) in mind, these materials releasing a dose of this drug more easily.

The composition of the pharmaceutical powder of course is quite optional and the powder may for instance comprise a pure active substance, a mixture of different active substances or a mixture of active substance(s) with adjuvant(s). It should be pointed out that the scope of choice of drugs is widened considerably due to the moisture-proof containment of the drug in the powder compartment.

The inhaler may be manufactured in the following way. A series of half-spherical indentations are formed in a strip of laminated aluminium foil in order to shape powder compartments. If the indentations are to be provided with through-holes, these are also formed at this stage. The indentations are filled with drugs and are topped off by means of scrapers, which will ensure a substantially uniform size of the different doses. An aluminium tape laminated with plastic is then welded over each indentation and around the indentation on the outside of the lower part.

The lower parts are then welded to upper parts and the strip is cut to form individual inhalers which are ready for packaging and use. The upper parts are moulded from sheets of plastic. In the moulding procedure care should be taken to ensure that the side walls of the upper part are as perpendicular as possible relative to the upper side in order to ensure an air flow which is as uniform as possible throughout the entire cross-section of the inhaler. The function of the abutments 10 primarily are to prevent that the ridge forming the constriction is distorted during the welding process.

Possible modifications of the invention.

The invention of course can be modified in many ways within the scope of the appended claims.

Thus the ridge 9 forming the constriction can be designed in different ways in order to enhance the lifting action of the air flow on the powder. Some examples thereof can be found in Figs 5 - 7.

Fig 5 illustrates how the ridge 9 can be provided with a small hole 26 centrally above the powder compartment

3. When the patient inhales through the inhaler, additional air will be directed more or less perpendicularly down into the powder compartment, thus enhancing the turbulent action in the vicinity of the powder compartment.

Figs 6 and 7 illustrate two alternative embodiments wherein the ridge has been provided with an edge 27 resp 28 oriented along the longitudinal extent of the ridge and which also will direct some air flow more directly into the powder compartment.

These embodiments will however require a higher degree of precision in the manufacturing in order to obtain the desired effect than the embodiment described above and will therefore be more difficult to manufacture.

The ridge 9 forming the constriction has been illustrated as being generally trapezoid in cross-section and as being generally rectilinear in longitudinal section. It should however be pointed out that the constriction may be shaped in many different ways within the scope of the appended claims.

The powder compartment can of course have another shape than a half-spherical shape and may for instance be elliptical, the minor axis thereof being parallel with the direction of the air flow, or may be otherwise trough-shaped. It is of course also possible to have several indentations, for instance if it is desired to increase the dose in an exactly defined way. As mentioned above, the powder compartment can be designed without the hole(s) 24. Two separate tapes furthermore can be used to seal the recess 3 respectively the hole(s) 24.

The projections 7,8 can be shaped otherwise than

conically and may for instance be shaped such that they direct a greater part of the air flow more directly past the powder compartment. They also could be integrated with the abutments 10.

5

The tape 6 could also be arranged in such a manner that it can be removed entirely from the lower part 2. In this case the projections 7,8 are not needed, at least not for the purpose of guiding and holding the tape.

10

The deaggregation means can be designed in other ways than in the form of planar surfaces oriented at an angle of about 20° - 50° relative to the direction of the air flow. This angle can of course also be varied outside this range and the surfaces do not necessarily have to be planar.

15

The material in the lower part and the tape does not necessarily have to comprise aluminium and may be any plastic material having the necessary impermeability and stiffness or having been treated to have these properties.

20

It is also conceivable to make the inhaler from a single sheet which is rolled or folded after having been moulded in an appropriate way.

25

CLAIMS.

1. Disposable breath-actuated inhaler comprising a
5 tubular housing forming an air flow path being open at
both ends, one end forming an air inlet (4) and one end
forming an air outlet (5), said housing comprising a
compartment (3) for storing a pharmaceutical powder to
be inhaled, c h a r a c t e r i z e d in that the
10 compartment (3) for storing the pharmaceutical powder
is located close to the air inlet (4) and is covered by
a thin foil (6) sealing the compartment in an airtight
way which can be removed from the compartment from
outside the housing, said housing being shaped with a
15 constriction (9) adjacent the powder compartment (3)
such that a turbulent air stream will be obtained at
the constriction upon inhalation which will lift the
powder out from the compartment (3) and mix the powder
into the air stream.

20

2. Inhaler according to claim 1, c h a r a c t e r i z e d in that said powder compartment (3) is connected
to the ambient air in its deepest part by means of one
or several through-holes (24).

25

3. Inhaler according to claim 1,
c h a r a c t e r i z e d in that said housing is
formed of two main parts, one moulded upper half (1)
and one generally flat lower half (2) having an
30 indentation (3) forming the powder compartment, said
~~two halves (1, 2)~~ being joined together along their
longitudinal sides.

4. Inhaler according to anyone of claims 1 to 3,
35 c h a r a c t e r i z e d in that the upper part (1)
is moulded from a thin sheet, preferably of plastics
material.

5. Inhaler according to claim 4,
c h a r a c t e r i z e d in that said constriction
(9) is formed as a depression in the upper side of
said upper part (1) which is oriented transversely
5 relative to the longitudinal extent of the tubular
housing and located above the powder compartment (3)
formed in the lower half (2) of the housing.

6. Inhaler according to any one of the preceding
10 claims, c h a r a c t e r i z e d in that the lower
half (2) is made of aluminium foil laminated with
plastic.

7. Inhaler according to any one of the preceding
15 claims, c h a r a c t e r i z e d in that the thin
foil is in the shape of a tape (6) having one free end
extending out through the air inlet (4), said tape
being attached around the edges of the powder
compartment (3) by means of relatively weak welds (22).

20

8. Inhaler according to claim 7,
c h a r a c t e r i z e d in that the inner end of the
tape (6) is attached to the lower half (4) between the
air inlet (4) and the powder compartment (3), the tape
25 (6) extending past, and being attached around, the
powder compartment (3), the tape then being bent
backwards about so as to extend out through the air
inlet (4).

9. Inhaler according to claim 8,
30 c h a r a c t e r i z e d in that the weak welds (22)
form a point facing downstream in order to facilitate
the initiation of the tearing action along the welds
(22) when the tape (6) is to be pulled out through the
35 air inlet (4) in order to expose the powder.

10. Inhaler according to any one of claims 7 - 9,

c h a r a c t e r i z e d in that projections (7, 8) extend downwards from the upper half (1) between the powder compartment (3) and the air inlet (4) for holding the tape (6) against the lower half (2) of the housing in order to prevent the tape (6) from obstructing the air flow path.

11. Inhaler according to any one of the preceding claims, c h a r a c t e r i z e d in that deaggregation means (11, 12, 13, 14, 15, 16) are located in the air flow path between the powder compartment (3) and the air outlet (5).

12. Inhaler according to claim 11, c h a r a c t e r i z e d in that said deaggregation means comprise planar surfaces (11, 12, 13, 14, 15, 16) oriented 20° - 50° , preferably 25° - 35° , most preferably 30° , relative to the longitudinal direction of the tubular housing, said surfaces being disposed generally perpendicularly to a plane through the longitudinal axis of the tubular housing, a projection of the planar surfaces onto a cross-section of the housing substantially covering said cross-section.

1/3

Fig. 1


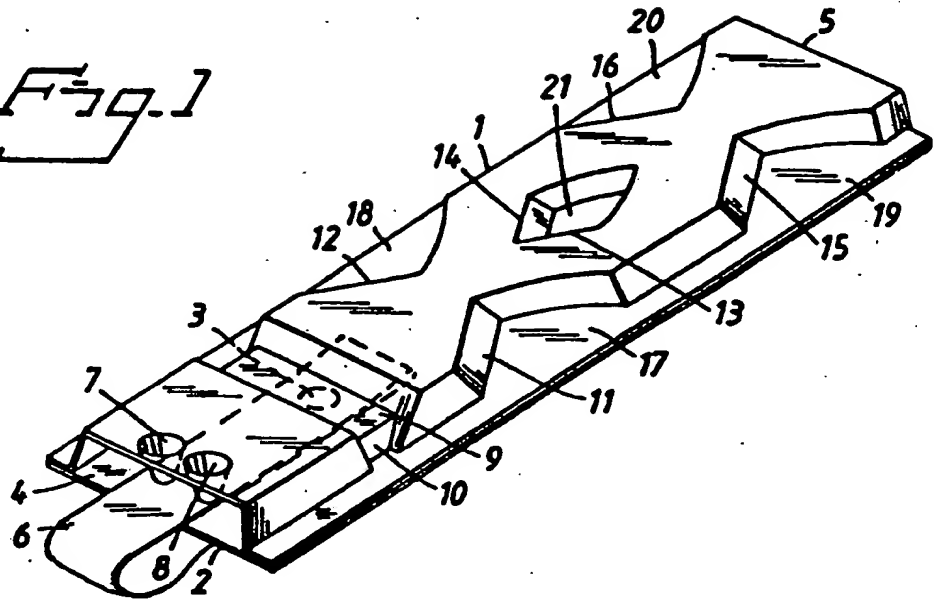


Fig. 2

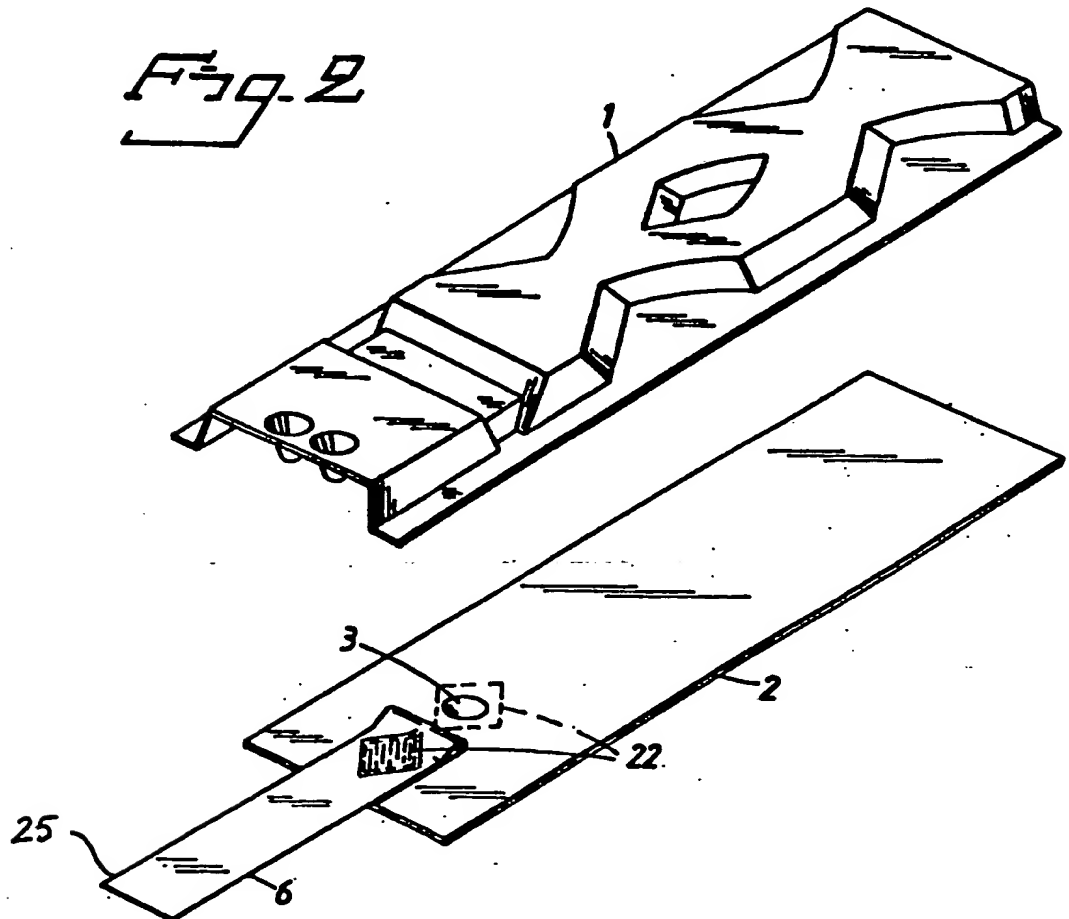

2/3

Fig. 3A

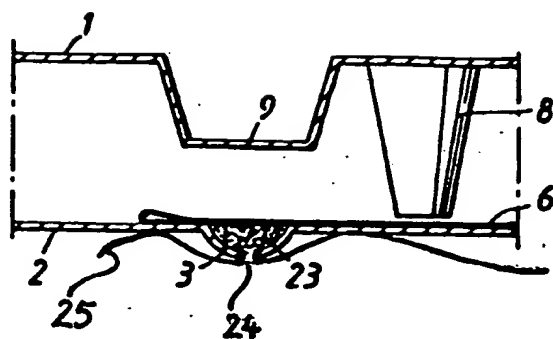


Fig. 3B

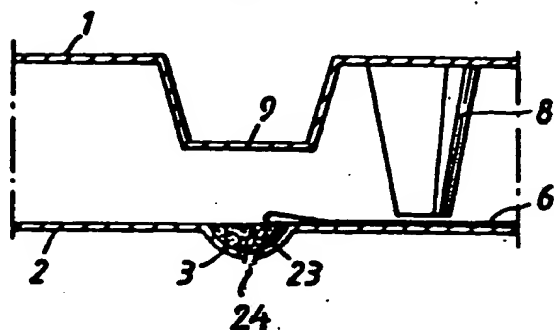


Fig. 3C


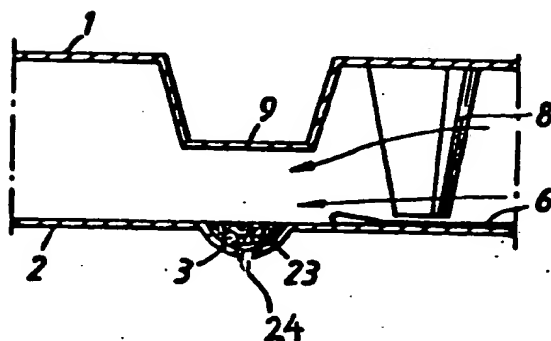


Fig. 4

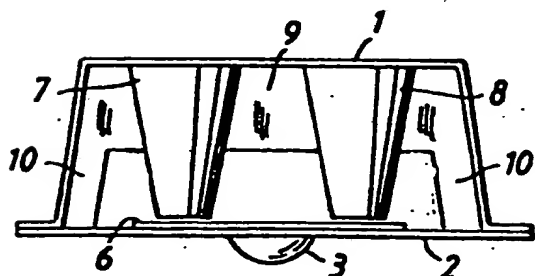

3/3

Fig. 5

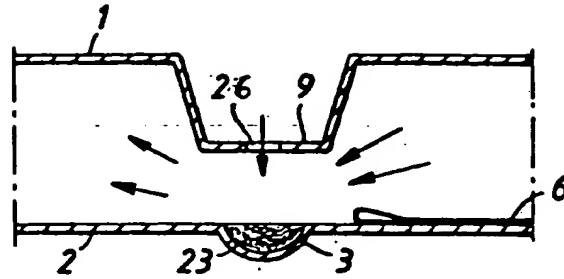


Fig. 6


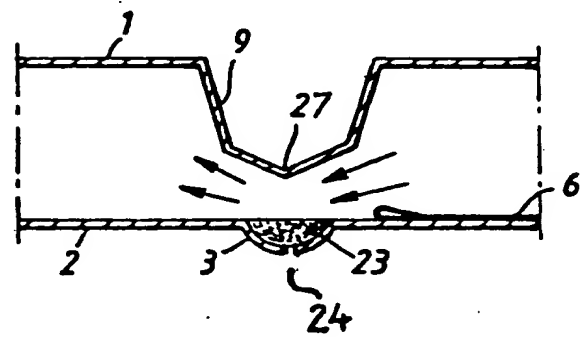


Fig. 7

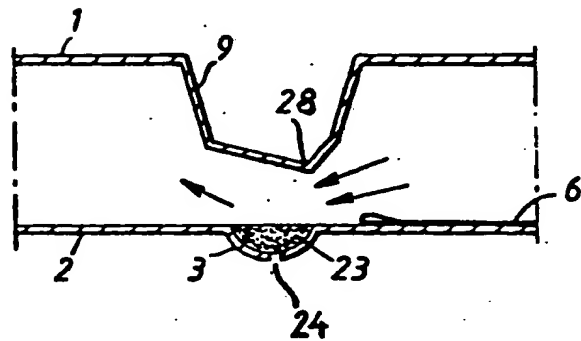

INTERNATIONAL SEARCH REPORT

International Application No

PCT/EP 93/00473

I. CLASSIFICATION OF SUBJECT MATTER (If several classification symbols apply, indicate all) ⁶ According to International Patent Classification (IPC) or to both National Classification and IPC Int.Cl. 5 A61M15/00																				
II. FIELDS SEARCHED <div style="text-align: center; border-top: 1px solid black; border-bottom: 1px solid black; margin: 5px 0;">Minimum Documentation Searched⁷</div> <table style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 30%; border-bottom: 1px solid black; padding: 5px;">Classification System</td> <td style="border-bottom: 1px solid black; padding: 5px;">Classification Symbols</td> </tr> <tr> <td style="padding: 5px;">Int.Cl. 5</td> <td style="padding: 5px;">A61M</td> </tr> </table> <div style="text-align: center; border-top: 1px solid black; border-bottom: 1px solid black; margin: 5px 0;">Documentation Searched other than Minimum Documentation to the Extent that such Documents are Included in the Fields Searched⁸</div>			Classification System	Classification Symbols	Int.Cl. 5	A61M														
Classification System	Classification Symbols																			
Int.Cl. 5	A61M																			
III. DOCUMENTS CONSIDERED TO BE RELEVANT⁹ <table style="width: 100%; border-collapse: collapse;"> <tr> <th style="width: 10%; border-bottom: 1px solid black; padding: 5px;">Category ¹⁰</th> <th style="width: 70%; border-bottom: 1px solid black; padding: 5px;">Citation of Document, ¹¹ with indication, where appropriate, of the relevant passages ¹²</th> <th style="width: 20%; border-bottom: 1px solid black; padding: 5px;">Relevant to Claim No.¹³</th> </tr> <tr> <td style="text-align: center; vertical-align: top; padding: 5px;">A</td> <td style="padding: 5px;">EP,A,0 404 454 (FISONS PLC) 27 December 1990 cited in the application see column 4, line 16 - line 46; figures ---</td> <td style="text-align: center; vertical-align: top; padding: 5px;">1</td> </tr> <tr> <td style="text-align: center; vertical-align: top; padding: 5px;">A</td> <td style="padding: 5px;">US,A,4 265 236 (PACELLA) 5 May 1981 cited in the application see abstract; figure 2 ---</td> <td style="text-align: center; vertical-align: top; padding: 5px;">1</td> </tr> <tr> <td style="text-align: center; vertical-align: top; padding: 5px;">A</td> <td style="padding: 5px;">WO,A,8 901 348 (TEIJIN LTD) 23 February 1989 cited in the application see abstract; figures 5-8 ---</td> <td style="text-align: center; vertical-align: top; padding: 5px;">1</td> </tr> <tr> <td style="text-align: center; vertical-align: top; padding: 5px;">A</td> <td style="padding: 5px;">US,A,5 042 472 (BUNIN) 27 August 1991 see abstract; figures 1-4 ---</td> <td style="text-align: center; vertical-align: top; padding: 5px;">1</td> </tr> <tr> <td colspan="3" style="text-align: center; padding: 5px;">-/--</td> </tr> </table> <div style="font-size: small; padding: 5px;"> <div style="display: flex; justify-content: space-between;"> <div style="width: 45%;"> <p>¹⁰ Special categories of cited documents :</p> <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier document but published on or after the international filing date</p> <p>"I" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p> </div> <div style="width: 45%;"> <p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step</p> <p>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.</p> <p>"&" document member of the same patent family</p> </div> </div> </div>			Category ¹⁰	Citation of Document, ¹¹ with indication, where appropriate, of the relevant passages ¹²	Relevant to Claim No. ¹³	A	EP,A,0 404 454 (FISONS PLC) 27 December 1990 cited in the application see column 4, line 16 - line 46; figures ---	1	A	US,A,4 265 236 (PACELLA) 5 May 1981 cited in the application see abstract; figure 2 ---	1	A	WO,A,8 901 348 (TEIJIN LTD) 23 February 1989 cited in the application see abstract; figures 5-8 ---	1	A	US,A,5 042 472 (BUNIN) 27 August 1991 see abstract; figures 1-4 ---	1	-/--		
Category ¹⁰	Citation of Document, ¹¹ with indication, where appropriate, of the relevant passages ¹²	Relevant to Claim No. ¹³																		
A	EP,A,0 404 454 (FISONS PLC) 27 December 1990 cited in the application see column 4, line 16 - line 46; figures ---	1																		
A	US,A,4 265 236 (PACELLA) 5 May 1981 cited in the application see abstract; figure 2 ---	1																		
A	WO,A,8 901 348 (TEIJIN LTD) 23 February 1989 cited in the application see abstract; figures 5-8 ---	1																		
A	US,A,5 042 472 (BUNIN) 27 August 1991 see abstract; figures 1-4 ---	1																		
-/--																				
IV. CERTIFICATION <table style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 50%; border-bottom: 1px solid black; padding: 5px;"> Date of the Actual Completion of the International Search <div style="text-align: center;">12 1993</div> </td> <td style="width: 50%; border-bottom: 1px solid black; padding: 5px;"> Date of Mailing of this International Search Report <div style="text-align: center;">20. 08. 93</div> </td> </tr> <tr> <td style="border-bottom: 1px solid black; padding: 5px;"> International Searching Authority <div style="text-align: center;">EUROPEAN PATENT OFFICE</div> </td> <td style="border-bottom: 1px solid black; padding: 5px;"> Signature of Authorized Officer <div style="text-align: center;">VILLENEUVE J.M.</div> </td> </tr> </table>			Date of the Actual Completion of the International Search <div style="text-align: center;">12 1993</div>	Date of Mailing of this International Search Report <div style="text-align: center;">20. 08. 93</div>	International Searching Authority <div style="text-align: center;">EUROPEAN PATENT OFFICE</div>	Signature of Authorized Officer <div style="text-align: center;">VILLENEUVE J.M.</div>														
Date of the Actual Completion of the International Search <div style="text-align: center;">12 1993</div>	Date of Mailing of this International Search Report <div style="text-align: center;">20. 08. 93</div>																			
International Searching Authority <div style="text-align: center;">EUROPEAN PATENT OFFICE</div>	Signature of Authorized Officer <div style="text-align: center;">VILLENEUVE J.M.</div>																			

III. DOCUMENTS CONSIDERED TO BE RELEVANT (CONTINUED FROM THE SECOND SHEET)		
Category *	Citation of Document, with indication, where appropriate, of the relevant passages	Relevant to Claim No.
X, P	WO, A, 9 204 069 (ASTRA AG) 19 March 1992 see the whole document -----	1, 3-12

**ANNEX TO THE INTERNATIONAL SEARCH REPORT
ON INTERNATIONAL PATENT APPLICATION NO.**

EP 9300473
SA 75292

This annex lists the patent family members relating to the patent documents cited in the above-mentioned international search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information. 12/08/93

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
EP-A-0404454	27-12-90	CA-A- 2019385	21-12-90
		JP-A- 3037077	18-02-91
US-A-4265236	05-05-81	None	
WO-A-8901348	23-02-89	AU-B- 608895	18-04-91
		AU-A- 2269588	09-03-89
		DE-A- 3871131	17-06-92
		EP-A- 0328685	23-08-89
		JP-T- 2500172	25-01-90
US-A-5042472	27-08-91	EP-A- 0481666	22-04-92
		JP-A- 4259471	16-09-92
WO-A-9204069	19-03-92	AU-A- 8512691	30-03-92
		CA-A- 2090694	13-03-92
		EP-A- 0548166	30-06-93